AD_	

Award Number: DAMD17-00-1-0662

TITLE: Multi-Pulse Ultrasound Contrast Imaging for Improved

Breast Cancer Diagnosis

PRINCIPAL INVESTIGATOR: Flemming Forsberg, Ph.D.

CONTRACTING ORGANIZATION: Thomas Jefferson University

Philadelphia, Pennsylvania 19107

REPORT DATE: September 2001

TYPE OF REPORT: Annual

PREPARED FOR: U.S. Army Medical Research and Materiel Command

Fort Detrick, Maryland 21702-5012

DISTRIBUTION STATEMENT: Approved for Public Release;

Distribution Unlimited

The views, opinions and/or findings contained in this report are those of the author(s) and should not be construed as an official Department of the Army position, policy or decision unless so designated by other documentation.

# REPORT DOCUMENTATION PAGE

Form Approved OMB No. 074-0188

Public reporting burden for this collection of Information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing this collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington, VA 22202-4302, and to the Office of

Management and Budget, Paperwork Reduction Proje	ect (0704-0188), Washington, DC 20503			
1. AGENCY USE ONLY (Leave	2. REPORT DATE	3 REPORT TYPE AND		
blank)	September 2001	Annual(1 Sep 0	0 - 31 Aug	01)
4. TITLE AND SUBTITLE			5. FUNDING N	
Multi-Pulse Ultrasound C	ontrast Imaging for I	Improved Breast	DAMD17-00-	-1-0662
Cancer Diagnosis				
_				
6. AUTHOR(S)				
Flemming Forsberg, Ph.D.				
_			,	
		· <del></del>		
7. PERFORMING ORGANIZATION NA	ME(S) AND ADDRESS(ES)		8. PERFORMIN	G ORGANIZATION
Thomas Jefferson University			REPORT NU	MBER
Philadelphia, Pennsylvania 19107				
I magorpma, I omisyrvama 1910.				
E-Mail: forsberg@esther.rad.tju.edu				
E-Mail: forsberg@estrier.rad.ijd.edu				
9. SPONSORING / MONITORING AGE	NCV NAME(S) AND ADDRESS/F	8)	10 SPONSORI	NG / MONITORING
9. SPONSORING/ MONITORING AGE	MCT MAME(S) AND ADDITESS(E	3)		EPORT NUMBER
U.S. Army Medical Research and M	Material Command			
Fort Detrick, Maryland 21702-501	2			
			<u> </u>	
11. SUPPLEMENTARY NOTES				
į				
12a, DISTRIBUTION / AVAILABILITY S	TATEMENT			12b. DISTRIBUTION CODE
Approved for Public Rele		limited		125. DIGITALDO HON CODE
Approved for Public Rele	sase; Discribation on	LIMICEG		
13. ABSTRACT (Maximum 200 Words	;)			
Preliminary reports	indicate that ult	rasound contras	st signific	cantly improves the
sensitivity and specifi	city of breast ultra	sound imaging.	We propo	se using a patented
multi-pulse contrast im	aging technique. Th	is technique an	oplies two	acoustic fields one
for bubble excitation a	and the other for image	aging The exc	itation fi	eld will momentarily
increase bubble sizes r	and the other for improve			
increase pubble sizes r	esurcing in an increa	/accord/ imagin	a field	If the imaging field
to the resonance size of	orresponding to the	(second) imaging		
is applied simultaneou	usly with (or sligh	itly after) th	e excitati	on rieid, acoustic
scattering from bubbles	around resonance si:	ze becomes mark	edly strong	ger than without the

modes, by developing multi-pulse contrast specific imaging.

To date, an in vitro dual-transducer pulse-echo system has been built to evaluate excitation enhanced imaging and initial experiments have been conducted with the contrast agents Sonazoid and Sonavist. Up to 12 and 16 dB improvement in SNR were measured in fundamental and second harmonic modes respectively. An NIH grant was submitted based on these preliminary results.

use in breast imaging with contrast agents, in conventional as well as harmonic imaging

This project will optimize the performance of ultrasound systems for

14. SUBJECT TERMS Breast Cancer, Ultraso	ound Imaging, Ultrasound Contrast Agent  15. NUMBER OF PA  10  16. PRICE CODE	16. PRICE CODE	
17. SECURITY CLASSIFICATION OF REPORT Unclassified	18. SECURITY CLASSIFICATION OF THIS PAGE Unclassified	19. SECURITY CLASSIFICATION OF ABSTRACT Unclassified	20. LIMITATION OF ABSTRACT Unlimited

excitation field.

# 3. TABLE OF CONTENTS

1.	FRONT COVER	1
2.	SF 298	2
3.	TABLE OF CONTENTS.	3
4.	INTRODUCTION	4
5.	BODY	4
	5.1 Methods	5
	S.D Reducto and Discussion	5
6.	KEY RESEARCH ACCOMPLISHMENTS	9
7.	REPORTABLE OUTCOMES.	9
8.	CONCLUSIONS	9
9.	REFERENCES	10

## 4. INTRODUCTION

The goal of any breast imaging modality is to improve the early detection of tumors and to improve the differentiation between benign and malignant lesions. While x-ray mammography is efficacious in diagnosing a high percentage of breast masses, it also produces a high rate of false positives [1]. The percentage of breast biopsies that are actually malignant vary between 10 % and 35 %. Thus, a technique that reliably differentiates between malignant and benign masses would improve the diagnosis of breast cancer and should, therefore, reduce the number of negative biopsies as well as the trauma of the patients. This proposal will attempt to establish such a technique through the novel and innovative use of multi-pulse ultrasound contrast imaging.

Ultrasound imaging is currently an auxiliary modality in breast imaging. It is mainly used to differentiate between cystic and solid lesions [2]. Investigations into the possibility of breast cancer diagnosis based on Doppler ultrasound flow detection have produced mixed results, due to overlap between flow measurements in benign and malignant tumors [3-4]. One problem may be the lack of sensitivity in flow detection in small tumor vessels using ultrasound. This hypothesis is supported by reports in the pathology literature describing angiogenic vascular morphology as an independent predictor of metastatic disease [5].

Ultrasound contrast agents produce increases of 15 to 25 dB in the echo intensities of blood flow signals; especially when combined with new contrast-specific imaging modalities such as harmonic imaging [6-7]. However, harmonic imaging has been found to suffer from reduced blood-to-tissue contrast resulting from second harmonic generation and accumulation in tissue. . Instead, we propose using a patented multi-pulse contrast imaging technique [8]. This technique applies two acoustic fields one for bubble excitation and the other for imaging. The excitation field will momentarily increase bubble sizes resulting in an increase in the number of bubbles with a size close to the resonance size corresponding to the (second) imaging field. If the imaging field is applied simultaneously with (or slightly after) the excitation field, acoustic scattering from bubbles around resonance size becomes markedly stronger than without the This project will optimize the performance of ultrasound systems for use in excitation field. breast imaging with contrast agents, in conventional as well as harmonic imaging modes, by developing multi-pulse contrast specific imaging based on Thomas Jefferson University's patented technology. The improved signal-to-noise ratio will enable clinicians to better depict breast tumor neovascularity and, thus, to better diagnose cancer.

Consequently, this project will examine approaches to and efficacy of inducing instantaneous bubble growth to momentarily enhance the backscattering from contrast microbubbles. This in turn should improve image contrast markedly and enable physicians to improve the diagnosis of breast cancer.

## **5. BODY**

The central hypothesis of this project is that the differentiation between benign and malignant breast lesions can be improved by using ultrasound contrast agents and excitation enhanced

imaging. To investigate this hypothesis excitation enhanced imaging will be investigated in vitro and then in vivo in rabbits with VX-2 tumors.

First an outline of the methods applied will be given followed by a presentation of the results to date. Finally, the conclusions and future directions of the research will be discussed.

#### 5.1 Methods

#### In Vitro experiments

To measure the shift in size of the microbubble population and, thus, the changes in backscattering of contrast microbubbles suspensions the experimental setup shown in Figure 1 in block diagram form was constructed. This system was based on the design of an active acoustic detector used by Roy and Apfel [9] for detecting microparticles with three transducers placed confocally in the same horizontally plane and immersed in a distilled water bath. The positioning of the transducers was guided with a 0.2 mm miniature needle hydrophone (Precision Acoustics Ltd, Dorchester, England).

The transducer within the excitation block produced a high-intensity (0.4, 0.8 and 1.2 MPa; average of peak positive and negative pressures) focused excitation ultrasound field. The acoustic pressure amplitude was calibrated using a PVDF needle hydrophone specifically designed to measure intensive ultrasound pressures (Imotec Messlehnik, Warendorf, Germany). The transducer was driven by a programmable arbitrary function generator (Model LW420, LeCroy Corporation, Chestnut Ridge, NY) through a 500W power amplifier (Model A-500, ENI, Rochester, NY). The frequency of the excitation transducer was chosen as either 0.528, 1.12 or 2.12 MHz to enable bubble growth [10], but at the same time to be within the bandwidth of current imaging transducers. Pulse lengths of 2, 16 and 128 cycles and pulse repetition frequencies (PRF's) of 2 and 20 Hz were investigated. A time modulus was used to synchronize the delay between the imaging and the excitation ultrasound pulses (varied from  $10-500~\mu s$ ). The key part of the modulus is a general-purpose lab pulse-delay generator (model AV-1023-C, Avtech Electosystems Ltd., Ogdensberg, NY).

A programmable function generator (Model 8116A; Hewlett Packard, Santa Clara, CA) produced pulses for transmission within the imaging block (Fig. 1). The transmit signals were first amplified in a broadband 50 dB RF power amplifier (Model 325LA; ENI, Rochester, NY) and then supplied to an acoustic transmit transducer. Signals scattered from contrast microbubbles were sensed by a receive transducer and amplified with a low noise RF amplifier (Model 5052 PR; Parametrics, Waltham, MA). The amplified signals were acquired at a sampling frequency of 25 MHz using a digital oscilloscope equipped with mathematical functions (Model 9350AM; LeCroy, Chestnut Ridge, NY). The command delivery to the function generator and the data transfer from the digital oscilloscope were controlled by LabView® (National Instruments, Austin, TX). The microbubble suspensions were diluted in Isoton® II (Coulter Corporation, Miami, FL) to around 0.02 μl of agent/ml of water and a magnetic stirrer was used to maintain mixture in a small waterbath instead (volume: 4.2 l).

#### 5.2 Results and Discussion

As originally proposed different types of contrast agents were studied. Time constraints and agent availability limited the study to two agents:

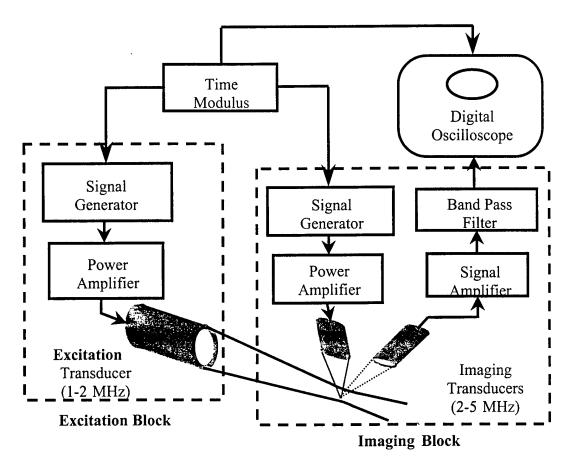


Figure 1. Block diagram of the experimental in vitro measurement system constructed.

- a) Sonazoid® (Nycomed-Amersham, Oslo, Norway), which is an encapsulated contrast agent containing a PFC gas.
- b) Sonavist® (Schering AG, Berlin, Germany), which consists of air microbubbles with a biodegradable shell composed of polybutyl-2-cyanoacrylate.

Initially, the enhancement obtained with excitation enhanced imaging relative to standard contrast imaging (i.e., the change in signal strength before and after the excitation pulse expressed in dB) was established as a function of the acoustic pressure employed in the excitation field. The PRF was either 2 Hz as in intermittent imaging or 20 Hz equivalent to real time. The excitation pulse length was 128 cycles and the imaging frequency and pressure were 3 MHz and 0.1 MPa, respectively. Marked improvements (approximately 10 dB) over regular contrast imaging was seen in intermittent mode, while the beneficial effects were less pronounced at 20 Hz PRF (on the order of 4 dB). This reduction in the efficacy of excitation enhanced imaging at the higher PRF is most likely due to the bubble destruction associated with real time imaging [11].

We also investigated whether the 10 dB enhancement seen at a 2 Hz PRF could be caused by bubble destruction from the excitation pulse itself. If that was the case, it should be possible to duplicate the results by increasing the acoustic pressure of the imaging pulse (i.e., as in intermittent imaging). Table 1 presents the results of increasing the imaging pulse pressure from 0.1 to 0.8 MPa at a 2 Hz PRF. Higher pressures were not possible without damaging the imaging transducer. The excitation pulse used in conjunction with the imaging had a 1.12 MHz center frequency and a pulse length of 16 cycles. The imaging frequency was 3.3 MHz. Clearly, even for a 0.8 MPa imaging pulse excitation enhanced imaging provided an additional 4 dB of enhancement. This proves that the enhancement observed with excitation enhanced contrast imaging is caused not merely by bubble destruction but, as predicted, by bubble growth.

To further substantiate the occurrence of bubble growth in excitation enhanced imaging we employed a high frequency (25 MHz), active acoustic detector developed by our group. Essentially this is the setup of Figure 1 with the two confocally placed imaging probes replaced by 25 MHz transducers (one for transmitting and one for receiving, as shown in the Imaging Block in Fig.1). The resolution of the active acoustic cavitation detector combined with the contrast microbubble concentration allows individual bubbles to be studied [12]. Figure 2a depicts ten sequences received with the 25 MHz transducer without any excitation pulse (pulse repetition interval 50  $\mu$ s). Clearly, this signal and thus, the bubble, remained unchanged over the measurement time 450  $\mu$ s (corresponding to the inter-pulse delays investigated). Conversely, Figure 2b shows the effect of firing a 2.5-MHz excitation pulse during the second sequence (notice the 2.5 MHz modulation from the excitation pulse superimposed on the 25 MHz detection pulse). The bubble size (indicated by the signal amplitude in sequences 3 – 10) is markedly larger following the excitation pulse (compare sequences 3 – 10 to sequence 1). This unequivocally proves that bubble growth occurs in excitation enhanced contrast imaging.

The effect of pulse length on the efficacy of excitation enhanced contrast imaging was limited. Even though the excitation pulse was varied from 2 to 128 cycles in length the enhancement did not change (given the approximately 2 dB standard deviation of the measurements). Likewise, we found that the effect of changing the delay between the excitation pulse and the imaging pulse from 10 to 500 µs was minimal.

Table 1. Enhancement in dB produced by excitation enhanced contrast imaging with Sonazoid for different imaging as well as excitation pulse pressures.

Excitation pulse Pressure [MPa]	Ima	aging pulse pressure [M	[Pa]
. ,	0.1	0.4	0.8
0.4	5.0	2.5	
0.8	8.0	5.0	4.0
1.2	8.5	4.5	4.0

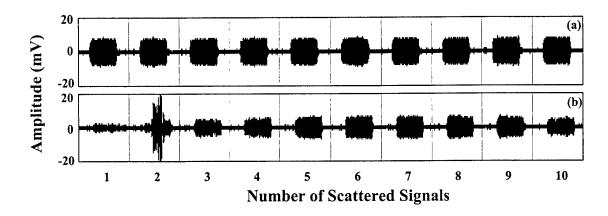


Figure 2. Sonazoid bubble (a) detected over 450 µs without excitation (and without bubble growth) and (b) demonstrating growth following a 2.5 MHz, 16 cycle 1.8 MPa excitation pulse. The imaging pulse pressure was less than 0.1 MPa in both cases. Notice, the difference in the initial bubble size (sequence 1) in the two cases.

Experiments were conducted, as mentioned, with the contrast agents Sonazoid and Sonavist, which produced an average enhancement following the excitation pulse on the order of 8 to 10 dB (for the optimal imaging parameters). These results all pertain to fundamental imaging. The same experiments were conducted for second harmonic imaging, where we found similar trends. The best results were obtained with Sonavist, which produced second harmonic enhancements up to 16 dB with an average of 13.4 dB (range 10 - 16 dB). An example of the change induced in Sonavist microbubbles by a 1.06-MHz excitation pulse is shown in Figure 3. Notice, there is even 8 dB of enhancement at the third harmonic (at 7.5 MHz). Sonazoid performed achieved enhancements at the second harmonic frequency ranging from 0 dB (in one case only) to 8 dB with an average of 4 dB. These results were presented at the annual meeting of the American Institute of Ultrasound in Medicine (AIUM) [13].

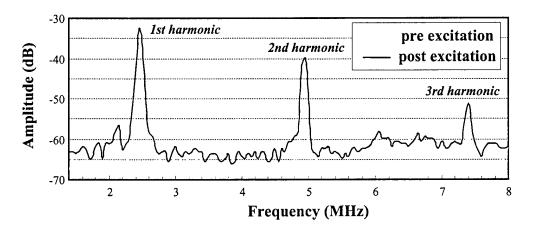


Figure 3. Sonavist spectra recorded with a 2.5 MHz low amplitude pulse (0.1 MPa) before and after a 1.06 MHz, 1.2 MPa, 16 cycle excitation pulse.

While the *in vitro* component of the project has been progressing, efforts have been hampered by the inability to recruit a student to work on the project and the *in vivo* component has not yet started. However, we have recently recruited a qualified candidate and, therefore, requested a one year no-cost extension. This extension will be utilized to complete the project. Nonetheless, the *in vitro* results were sufficiently encouraging that an NIH/SBIR grant entitled "System for Excitation Enhanced Ultrasound Contrast Imaging" was submitted using these results as preliminary data. We recently learned that this grant is being funded.

## 6. KEY RESEARCH ACCOMPLISHMENTS

- An in vitro system was built to evaluate excitation enhanced imaging.
- Initial experiments were conducted with Sonazoid and Sonavist.
- Optimal acoustical imaging parameters for excitation enhanced imaging were explored.
- Enhancement up to 10 dB and 16 dB was measured in fundamental and harmonic mode, respectively.

#### 7. REPORTABLE OUTCOMES

#### Manuscripts, abstracts, presentations

W. T. Shi, R. Bautista, F. Forsberg, C. Vecchio, R. Bernardi, B.B. Goldberg: Evaluation of excitation enhanced ultrasound contrast imaging. *J Ultrasond Med*, vol. 20, pp. S12, 2001.

March 11 - 14, 2001. The 45<sup>th</sup> Annual Convention of the American Institute of Ultrasound in Medicine, Orlando, FL, USA.

• Evaluation of excitation enhanced ultrasound contrast imaging.

#### Degrees and Grant submissions

NIH (SBIR), grant no R44 HL62830-02A1; System for Excitation Enhanced Ultrasound Contrast Imaging (subcontract to Spectrasonics Inc).

Raymond Ro has been employed on this project and is working towards his PhD degree in Biomedical Engineering (to be obtained from Drexel University) with F. Forsberg (the PI) as his supervisor.

#### 8. CONCLUSIONS

In summary, significant enhancement (up to 16 dB) has been achieved with excitation enhanced imaging *in vitro*, but due to the delay in hiring a student the project is approximately 6 months behind the original schedule.

# 9. REFERENCES

- 1. Feig SA: Breast masses: Mammographic and sonographic evaluation. *Radiologic Clin North Am* 30:67-92, 1992.
- 2. Jackson VP: The Role of US in Breast Imaging. Radiology, 177:305-311, 1990.
- 3. Bohm-Velez M, Mendelson EB: Computed tomography, duplex Doppler ultrasound and magnetic resonance imaging in evaluating the breast. *Semin Ultrasound CT MR*, 10:171-176, 1989
- 4. Adler DD, Carson PL, Rubin JM, Quinn-Reid D: Doppler ultrasound color flow imaging in the study of breast cancer: preliminary findings. *Ultrasound Med. Biol.*, 16: 553-559, 1990.
- 5. Weidner N, Folkman J, Pozza F, et al. Tumor angiogenesis: a new significant and independent prognostic indicator in early-stage breast cancer. *J Natl. Cancer Inst.*, 84: 1875-1887, 1992.
- 6. Forsberg F, Merton DA, Liu JB, Needleman L, Goldberg BB: Clinical applications of ultrasound contrast agents. *Ultrasonics*, 36: 695 701, 1998.
- 7. Goldberg BB, Raichlen JS, Forsberg F. *Ultrasound Contrast Agents: Basic Principles and Clinical Applications* (2<sup>nd</sup> Ed). Martin Dunitz Ltd., England, 2001.
- 8. Wu YQ, Forsberg F, Goldberg BB. Excitation enhanced ultrasound system. US patent # 5,833,615, 1998.
- 9. Roy RA, Apfel RE. Mechanical characterization of microparticles by scattered ultrasound. J Acoust. Soc. Am. 87, 2332-2341, 1990.
- 10. Flynn, HG, Church, CC. Transient pulsations of small gas bubble in water. J. Acoust. Soc. Am. 84, 985-998, 1988.
- 11. Porter TP, Xie F. Transient myocardial contrast after initial exposure to diagnostic ultrasound pressures with minute doses of intravenously injected microbubbles. *Circulation* 92, 2391-2395, 1995.
- 12. Shi WT, Forsberg F, Tornes A, Østensen J, Goldberg BB. Destruction of contrast microbubbles and the association with inertial cavitation. *Ultrasound Med. Biol.*, 26, 1009 1019, 2000.
- 13. W. T. Shi, R. Bautista, F. Forsberg, C. Vecchio, R. Bernardi, B.B. Goldberg: Evaluation of excitation enhanced ultrasound contrast imaging. *J Ultrasond Med*, 20, S12, 2001.